



## TARGET PROBE: HS-ICOS


ADVANCED CELL DIAGNOSTICS

### RNASCOPE® PROBE INFORMATION

<b>Catalog number:</b>	407141 (Manual)*, 407146 (VS assay)*, 407147 (LS assay)* 407149 (2.5 VS assay)*, 407148 (2.5 LS assay)*
<b>Species:</b>	Homo sapiens
<b>Target Gene:</b>	ICOS
<b>Alternate names:</b>	AILIM; CD278; CVID1
<b>Entrez Gene ID:</b>	29851
<b>Accession#:</b>	NM_012092.3
<b>Unigene:</b>	Hs.56247
<b>Target Sequence:</b>	Homo sapiens inducible T-cell co-stimulator (ICOS) mRNA
<b>Probe Region:</b>	651 - 1857
<b>ZZ pair number:</b>	20

\* Target region is the same across manual and automation

### PROBE DATA

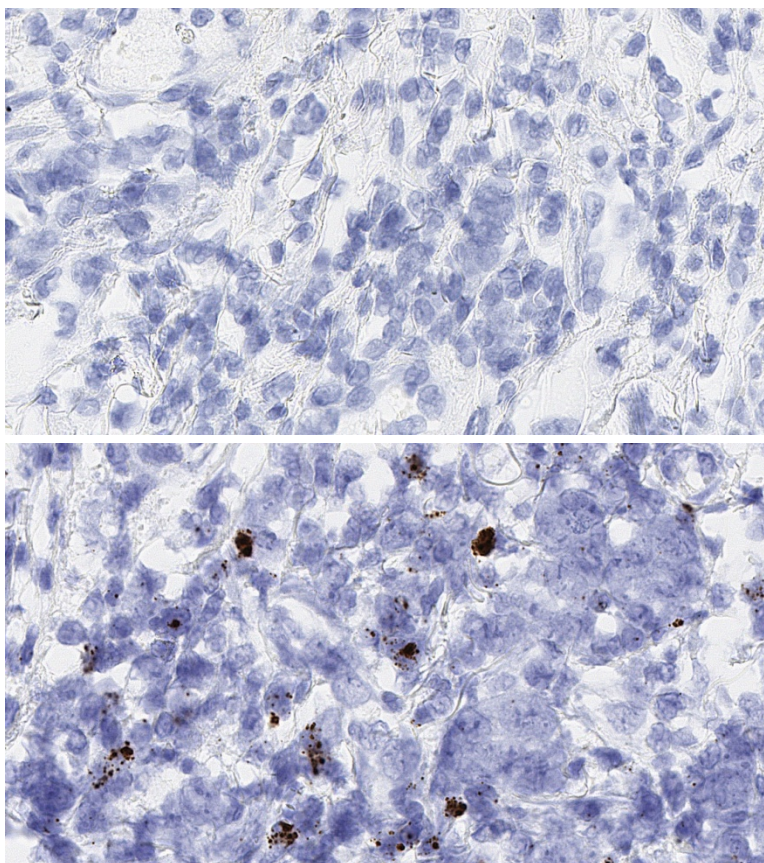

RNAscope® Manual Brown Assay performed on FFPE gastric cancer tissue under standard condition, using the dapB Negative Control probe (Top; Cat. No. 310043) and Hs-ICOS probe (Bottom; Cat. No. 407141), 40X

For more information regarding this target gene: <http://www.ncbi.nlm.nih.gov/gene/29851>

**Note:** ACD always recommends RNA quality verification using control probes, prior to running a target marker. Expression pattern may vary from data shown here based on tissue preparation methods and/or associated sample biology.