



TARGET PROBE: HS-HOTAIR


ADVANCED CELL DIAGNOSTICS

RNASCOPE® PROBE INFORMATION

Catalog number:	312341 (Manual)*, 312349 (2.5 VS assay)*, 312348 (2.5 LS assay)*
Species:	Homo sapiens
Target Gene:	HOTAIR
Alternate names:	HOXAS; HOXC-AS4; HOXC11-AS1; NCRNA00072; HOTAIR
Entrez Gene ID:	100124700
Accession#:	NR_047518.1
Unigene:	Hs.197076
Target Sequence:	Homo sapiens HOX transcript antisense RNA (HOTAIR), transcript variant 3, non-coding RNA
Probe Region:	602-2134
ZZ pair number:	30

* Target region is the same across RNAscope® manual and automation assays

PROBE DATA

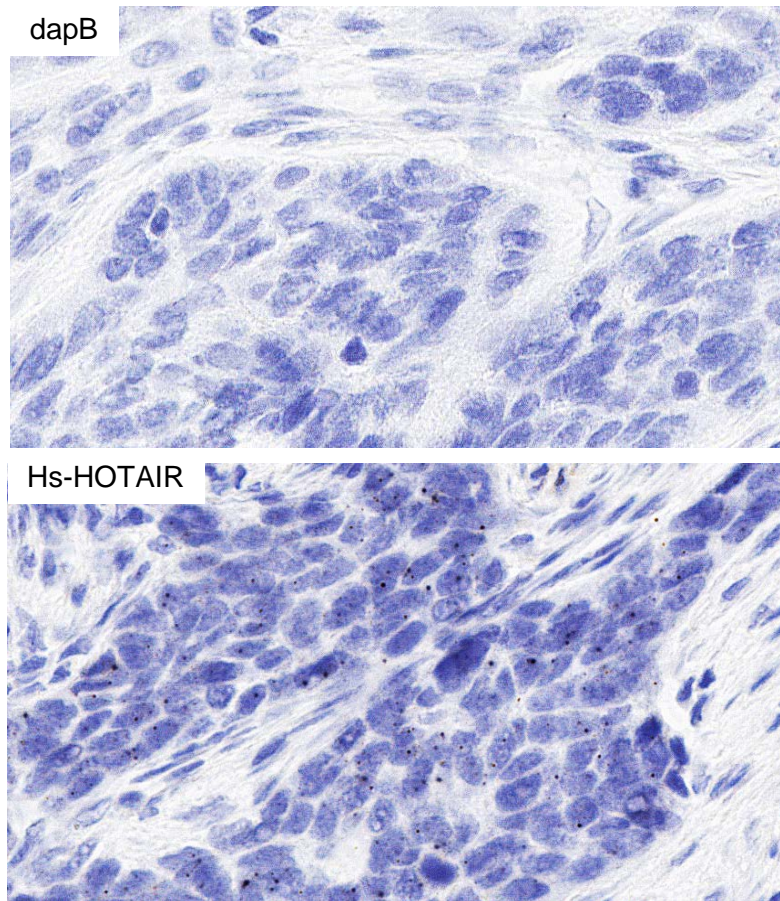

RNAscope® Manual Brown Assay performed on FFPE esophageal cancer tissue under standard condition, using the dapB Negative Control probe (Top; Cat. No. 310043) and Hs-HOTAIR probe (Bottom; Cat. No. 312341), 40X

For more information regarding this target gene: <http://www.ncbi.nlm.nih.gov/gene/100124700>

Note: ACD always recommends RNA quality verification using control probes, prior to running a target marker.

Expression pattern may vary from data shown here based on tissue preparation methods and/or associated sample biology.